

ScreenIT A30 Connect

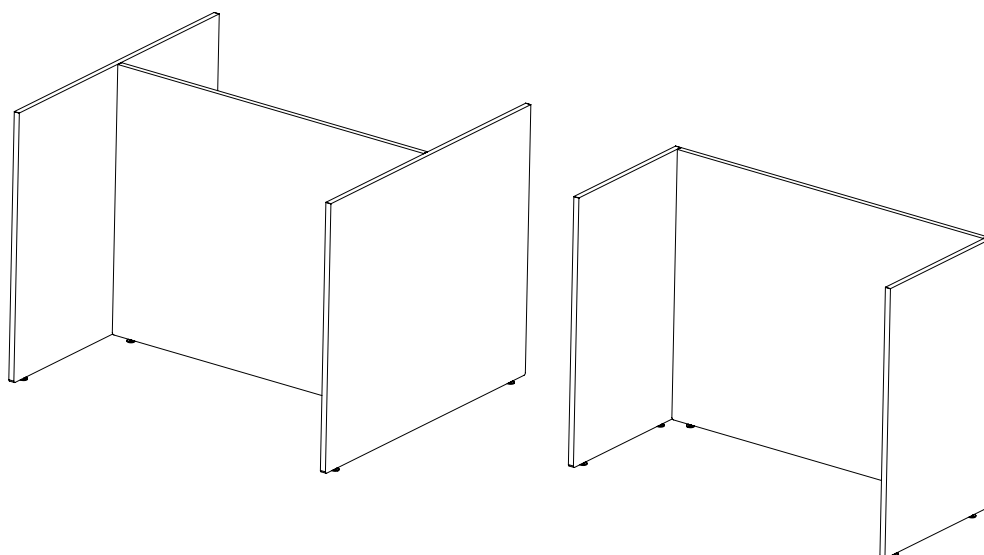


TABLE OF CONTENTS

General	2
Symbols	2
Tools	2
Care Instructions	2
Assembly instruction	3
Add booth	3
Disassembly instruction	4

GENERAL

Congratulations on your purchase of a Götessons Industri AB product!

In order to maximise the service life and to get the best quality, it is important to follow the installation instructions. Götessons disclaims all liability and warranty for damage caused by improper use or handling of the product that does not comply with the instructions in this manual. For warranty conditions, see our website.

For questions please contact Götessons.

SYMBOLS



Risk of compression of hands or other body parts.



Replaceable spare part
Contact Götessons



CAUTION: Contains magnets.
Maintain a minimum distance of 15 cm from pacemakers and ICDs to prevent potential interference.
NOTE! Only during assembly.



Looks may vary

TOOLS




CARE INSTRUCTIONS





Maximize life – minimize waste.
Follow this guide for correct repair and end-of-life disassembly. Proper handling ensures your warranty remains valid and enables 100% material recycling. Contact Götessons for spare parts or circularity inquiries.

ASSEMBLY INSTRUCTION

1)


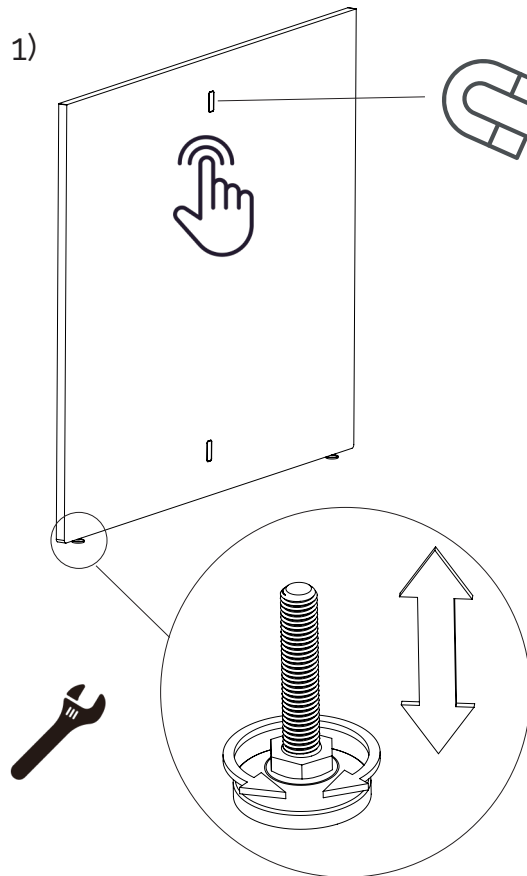


2)

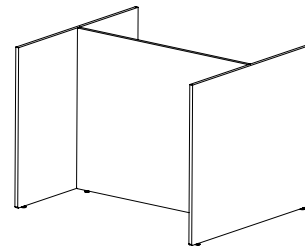
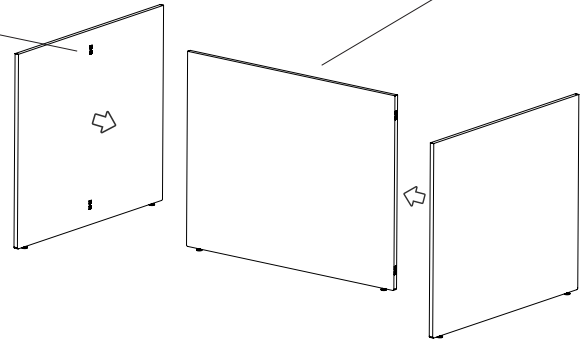


ADD BOOTH



1)





2)











3)

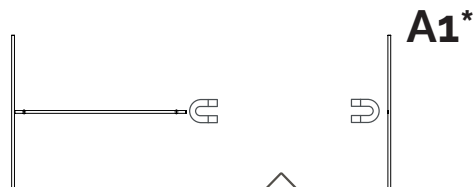

4)

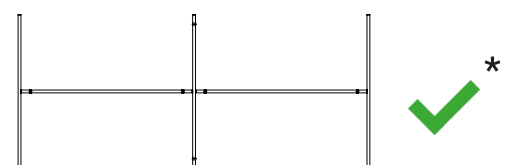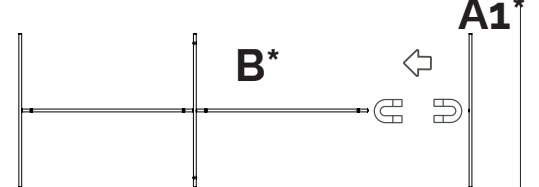

DISASSEMBLY INSTRUCTION

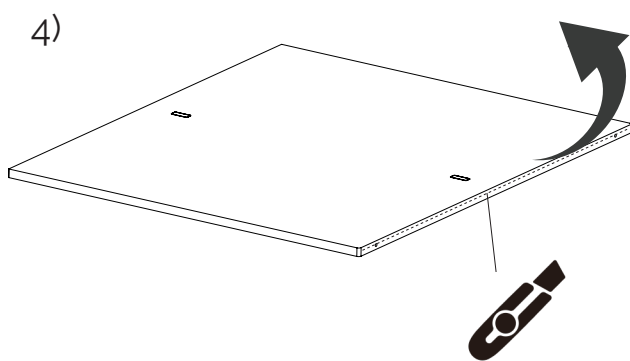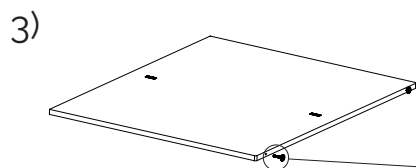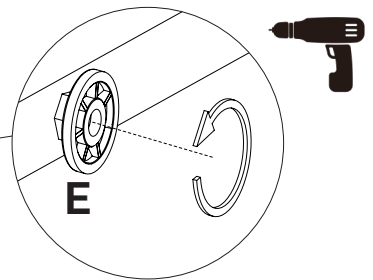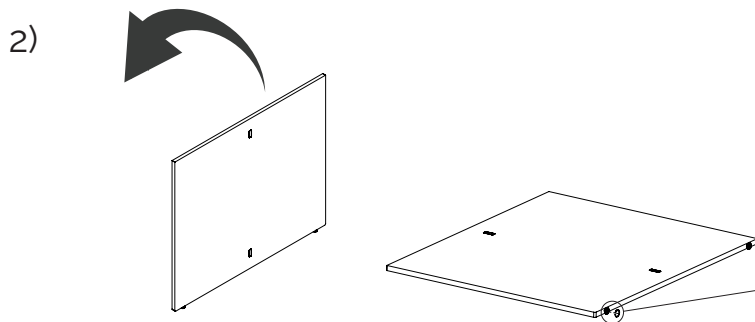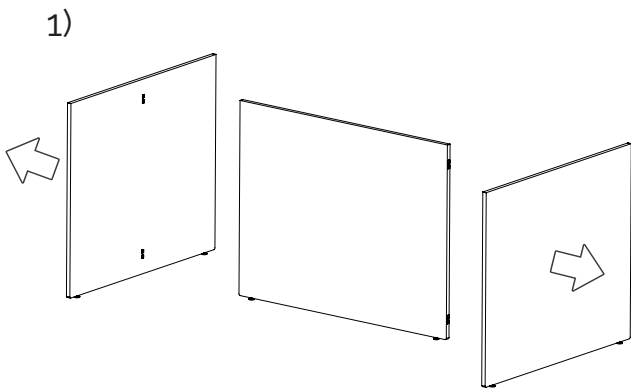

TOOLS

